
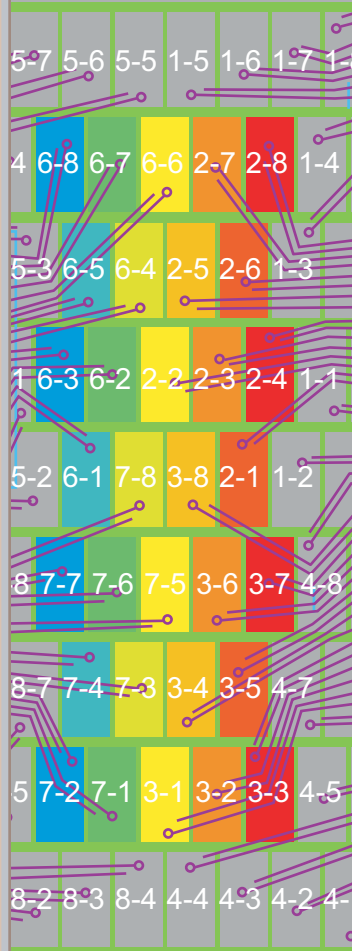


Cornell TPC event:
 track
 enters top-right
 exits center-left

ArCO2(10%)
 cage: -20kV
 @ termination: -900V
 grid: -600V
 pads: -2000V
 anode: +550V

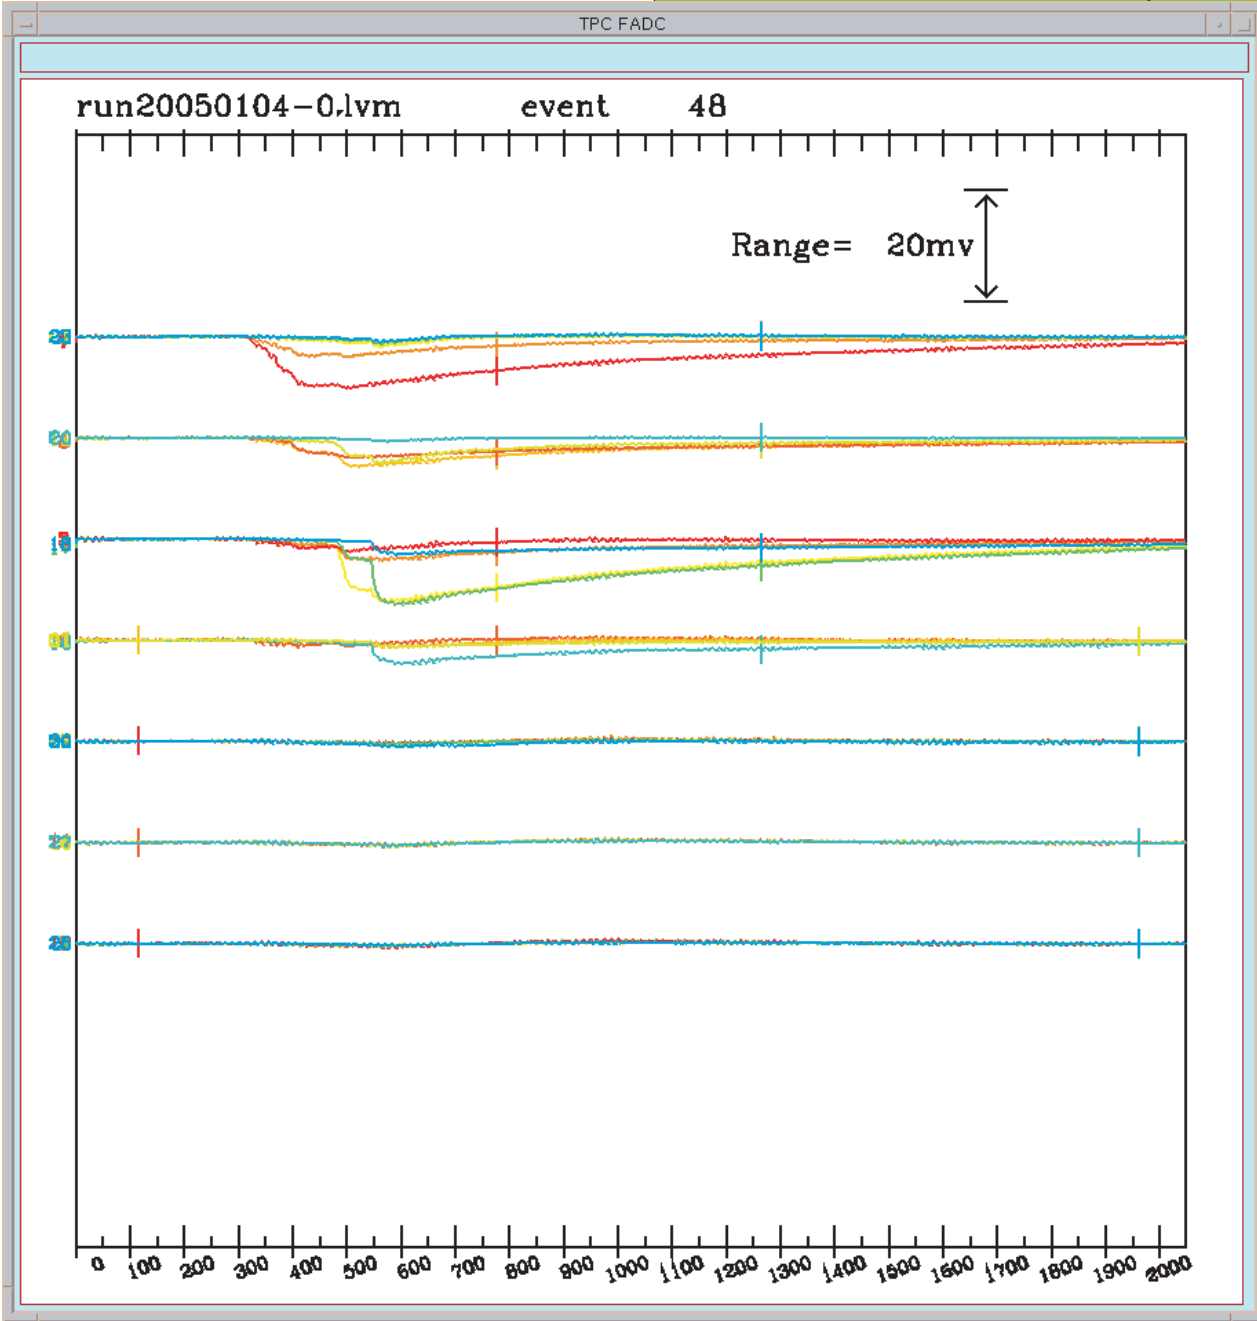

There are 7 instrumented pad rows on the readout board. The 32 pulse height spectra are offset in the display to correspond to the 7 pad rows; the color identifies the pad within the row.

2048 time buckets, 100MHz, 20.48 μ s